



Test Report/ Certificate of Analysis

Date of Report June 18, 2026

To: Research Only

From: AxisPharm, LLC

Certificate ID Number: 18Jun2026-29

Results reported by: Lab Technician
Ning Yang

Review/Approved by: 
QA Director
Dawei Yue

Sample Received: Date: 06/08/2026
Receiving Condition: ☒ Acceptable ☐ Other: _____
Storage Condition: ☐ Room temperature ☐ -20°C ☐ -80°C
☒ Other: __ 0 °C ____

Method(s): Sample Name: KLOW 80MG; Brand Name: Research Only;
Lot#: RO-KLOW806.1.2026; MFD: NA; BBD: NA
LCMS and LAL endotoxin Assay

Procedure(s): Laboratory Activity Date: 06/10/2026


Results:

AxisPharm, LLC

Results only apply to tested Research Use Only samples within Test Report as received. Not for use in humans or animals. Analytical data apply only to the batch tested and do not indicate suitability for diagnostic or therapeutic use. Any unauthorized alteration, reproduction, or relabeling of this COA renders it invalid.



Test Report/ Certificate of Analysis

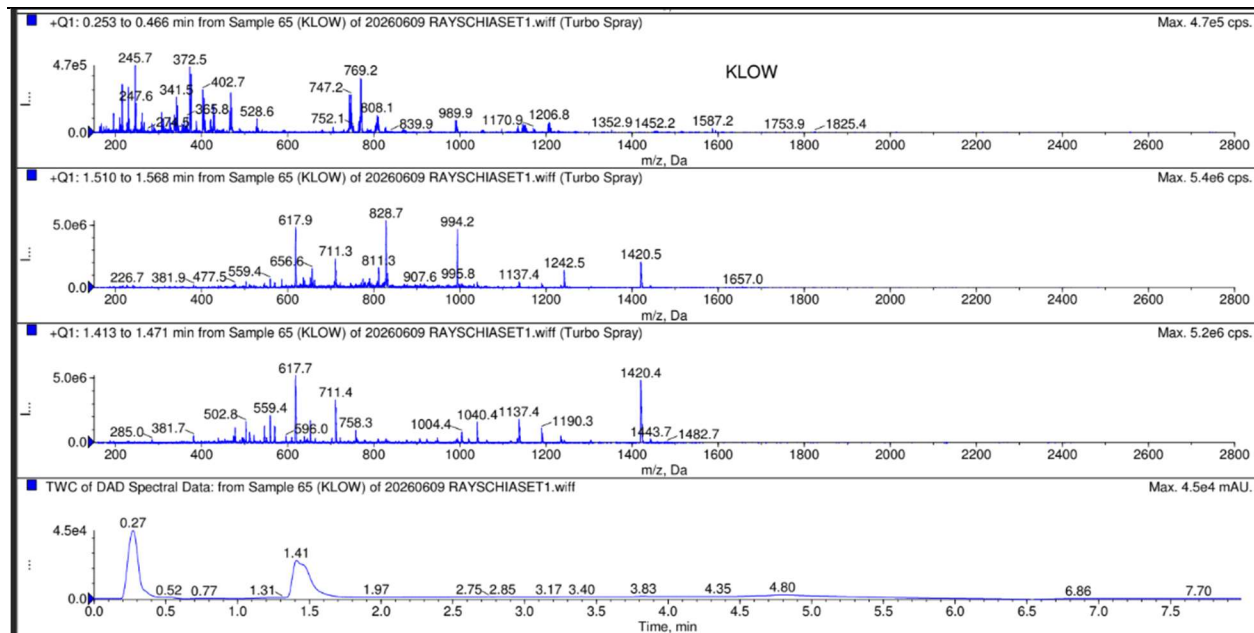

Sample Name	Net Weight Measured	MW (g/mol)	Detected	UV Purity (220nm) (%)
KLOW 80MG	76.3 mg	403.5/1419.5/ 4964.0/342.5	402.7/1420.5[M+H]; 1242.5[M+4H],994.2[M+5H]/343.2[M+H]	99.3

Endotoxin Results:

Sample Name	Endotoxin Testing Value (EU/mg)
KLOW 80MG	0.055

Salts and sugars that serves as fillers in injectables are not considered as impurities.

Conclusion: The product comes with KLOW 76.3MG with purity of 99.3%.